



**Project** 135558  
**Lab #** 131063  
**Date Rec'd** 12/9/2025  
**Report Issued** 12/23/2025

**Project**  
**Sample** Semax 10 mg

## Certificate of Analysis




<u>Analyte</u>	<u>Result</u>	<u>LOQ</u>	<u>Units</u>	<u>% of Label</u>	<u>Method</u>	<u>Date</u>	<u>CAS</u>
<b>Peptide Analysis</b>							
Chromatographic purity	99.94	0.5	%		HPLC-UV/MS	12/16/2025	
Semax	11.0	0.5	mg	110.0	HPLC-UV-MS	12/16/2025	80714-61-0
Semax	ID Confirmed				HPLC-UV-MS	12/16/2025	80714-61-0

The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.  
 Methods shown reference current Krause Analytical SOPs  
 ND - Not detected LOQ - limit of quantification  
 Copyright © 2025 Krause Analytical LLC. All rights reserved.

Respectfully submitted,


Mark C. Krause  
 Laboratory Director



krause analytical

### Chromatogram

Response\_

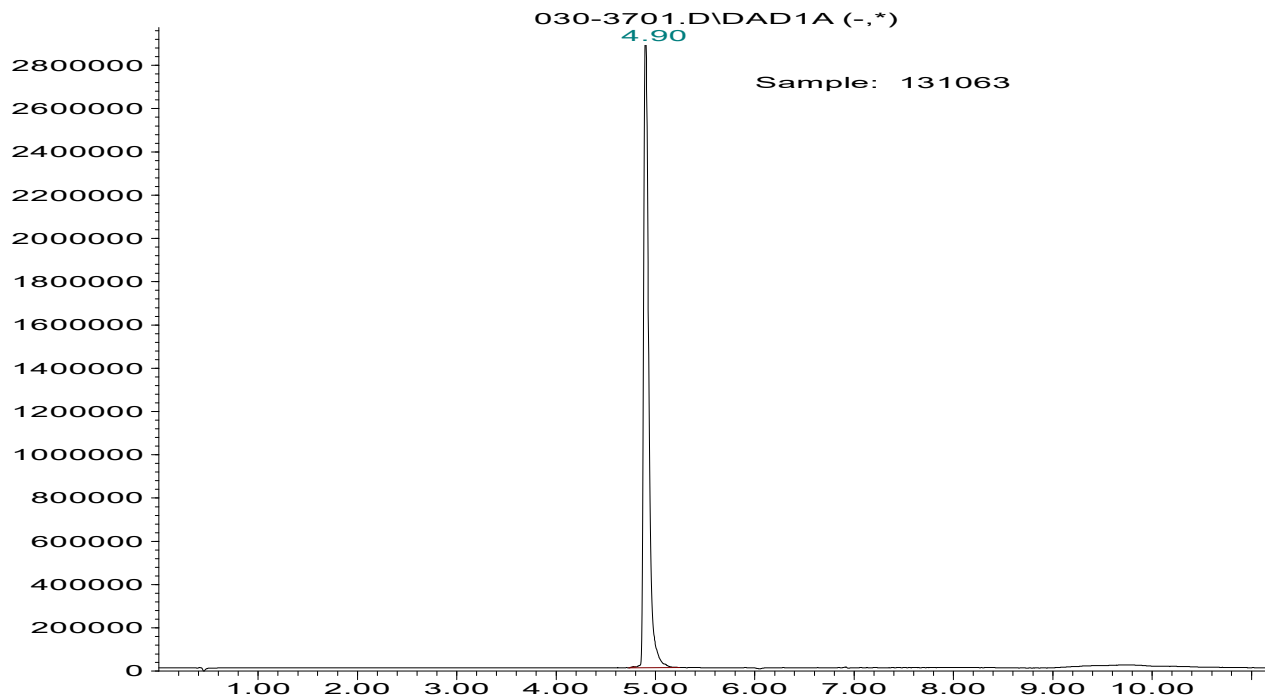

Time

### Mass spectrum/Reference Spectrum

